



Particulate Matter Testing

Eurofins BioPharma Product Testing is well-versed in testing particulate matter ranging from $<.01\ \mu\text{m}$ to $>3,000\ \mu\text{m}$ and uses a variety of techniques to develop and validate particle size methods. Our scientists are experienced in using orthogonal techniques to address a wide range of product and formulation issues—from protein aggregation through extraneous matter contamination.

Why Choose Eurofins BioPharma Product Testing?

- We offer a broad set of orthogonal methods covering the entire particle size range.
- Direct interaction with our technical staff will ensure a testing strategy appropriate for your product formulation.
- Our more than 30-year history of cGMP regulatory compliance ensures delivery of the highest quality data.

Dynamic and Static Light Scattering

Particle size and molecular size are measured at a 90 degree scattering angle using Dynamic Light Scattering. Zeta potential and electrophoretic mobility can also be measured using Laser Doppler Microelectrophoresis and molecular weight using Static Light Scattering.

Volume requirements: 0.1 g – 0.5 g per sample.

Particle sizes: $0.0003\ \mu\text{m}$ – $5\ \mu\text{m}$.

Instrumentation: Malvern Zetasizer Nano ZS90.

Quasi Elastic Light Scattering (QELS)

This test measures and uses molecular motion to determine the diffusion coefficient of a molecule in solution. The diffusion coefficient for a spherical particle is directly related to its “hydrodynamic radius.”

Volume requirements: Approximately 100 μg (i.e., 100 μL injection of 1 mg/mL solution for in-line SEC operation).

Particle Sizes: Approximately $0.0005\ \mu\text{m}$ – $.03\ \mu\text{m}$.

Instrumentation: WyattQELS, which is embedded within Wyatt HELEOS II.

Multi-Angle Light Scattering (MALS)

A static light scattering technique can be used in conjunction with Size Exclusion Chromatography (SEC) as an in-line detection technique, or it can be used for non-fractionated samples in the batch mode of operation.

Volume requirements: Approximately 100 μg (i.e., 100 μL injection of 1 mg/mL solution for in-line SEC operation) and 1,000 μg (Direct 1000 μL infusion of 1 mg/mL solution for batch mode operation).

Particle Sizes: $.01\ \mu\text{m}$ – $.5\ \mu\text{m}$.

Instrumentation: Wyatt Technologies HELEOS II.

Laser Light Diffraction

Particle size of a spherical particle is measured by the dispersion and absorption of light (scattering pattern) generated by a laser using either wet or dry dispersion techniques. A sample's scattering pattern is directly related to its particle size.

Volume requirements: 0.1 g – 0.5 g per sample for wet dispersion. 0.5 g – 5 g per sample for dry dispersion.

Particle sizes: $0.02\ \mu\text{m}$ – $600\ \mu\text{m}$ for wet dispersion and $0.02\ \mu\text{m}$ – $2,000\ \mu\text{m}$ for dry dispersion.

Instrumentation: Malvern Mastersizer 2000 with Hydro S wet dispersion and the Scirocco 2000 dry dispersion unit.

Micro Flow Imaging System (MFI)

Flow cell and digital photography are used to individually image, size, and count particles in liquid formulations. Using an autosampler or by manual injection, the sample is passed through the flow cell and pictures are captured after automatic illumination and precision focusing. MVSS software is used to process the captured images and determines the particle size and count within a desired particle size range. MVAS software is also used to identify the sample particle's morphology and shape attributes that traditional light obscuration (LO) and size exclusion chromatography (SEC) technologies are not able to detect.

Volume requirements:

1.0 – 2.0 mL per sample (5200 Model)

1.0 – 6.0 mL per sample (5100 Model)

Particle Sizes:

$1\ \mu\text{m}$ – $70\ \mu\text{m}$ (5200 with 100 μm flow cell)

$2\ \mu\text{m}$ – $300\ \mu\text{m}$ (5100 with 400 μm flow cell)

Instrumentation: Protein Simple MFI 5100 Micro Flow Imaging System (comprised of MFI 5100 Flow Microscope, MFI View System Software (MVSS) and MFI View Analysis Suite (MVAS) Software).

Light Obscuration Test

Based on the principle of light obscuration, this test allows for automatic determination of the size and number of particles according to their size. The test is performed in a biological safety cabinet, under conditions that limit foreign particulate matter.

Volume requirements:

USP <788>/EP 2.9.19/JP 6.07: A minimum of 25 mL pooled sample solution is required to meet the harmonized USP/EP/JP requirements. Dilutions of samples can be performed as required.

USP <787>: Can be used as an alternative to USP <788> and specifically addresses testing of therapeutic protein injections and related preparations. Smaller test volumes are allowed, and there is no specific volume requirement as compared to USP <788>. Specific



sample handling instructions take into account potential issues associated with analysis of these types of materials.

Particle sizes: The compendial requirement is to enumerate particles at $\geq 10 \mu\text{m}$ and $\geq 25 \mu\text{m}$, although particles in the range of $\geq 2 \mu\text{m}$ - $400 \mu\text{m}$ can also be enumerated.

Instrumentation: HIAC 9703+ Liquid Particle Counting System.

Microscopic Particle Count Test

Utilized when certain test articles cannot be analyzed by the Light Obscuration method due to color, reduced clarity and/or viscosity. This method can also be utilized in the event a product does not meet the USP criteria for the Light Obscuration Method.

Volume requirements: A minimum of 10 containers is required to meet USP/EP/JP requirements. An alternate number of containers can be analyzed and dilutions of samples can be prepared if warranted.

Particle sizes: The compendial requirement is to detect particles at $\geq 10 \mu\text{m}$ and $\geq 25 \mu\text{m}$. Particles $< 10 \mu\text{m}$ cannot be accurately detected using the Microscopic Method.

Instrumentation: Olympus BMAX BX60 microscope, equipped with an internal episcopic brightfield illuminator, a circular diameter graticule and an external focusable auxiliary illuminator.


Analytical Sieving

Sieving is usually the method of choice for classification of the coarser grades of single powders or granules. It is a particularly attractive method in that powders and granules are classified only on the basis of particle size, and in most cases, the analysis can be carried out in the dry state. Mechanical sieving is most suitable where the majority of the particles are larger than about $75 \mu\text{m}$. For smaller particles, other means of agitation such as air-jet sieving may be more appropriate.

Volume requirements: 10 g – 100 g is generally required per test. However, if the information needed to perform sieve testing for a specific material (i.e. sample amount, sieve sizes and sieve time) cannot be provided, then approximately 500 g will be required in order to perform feasibility/endpoint determination to establish the appropriate parameters prior to testing the material.

Particle sizes: Certified ISO 3310-1, ASTM E-11 sieves in sizes ranging from $25 \mu\text{m}$ to $2,000 \mu\text{m}$. Larger sizes up to 11.20 mm may be purchased upon request.

Instrumentation: Endecotts Octagon 200 Test Sieve Shaker, W.S. Tyler Model RX-29 Ro-Tap Shaker and Hosokawa Micron AirJet Sieve (Version II).

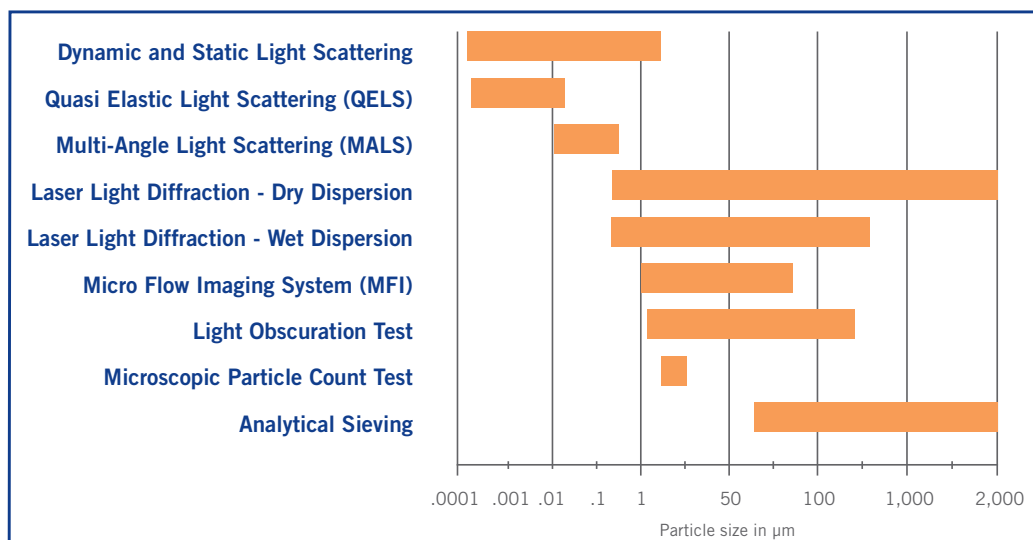

Comprehensive GMP Testing Services

Method Development & Validation • Release Testing • Raw Materials Testing
Cell Banking Services • Virology Services • Facility & Process Validation
Chemistry • Biochemistry • Molecular & Cell Biology • Microbiology
Stability Testing & Storage • Primary & Secondary Package Testing

Flexible Service Models

Fee For Service (FFS)
Full-Time-Equivalent (FTE)
Professional Scientific
Services® (PSS)

Global Facilities

Australia	Denmark	India	Japan	Spain	UK
Belgium	France	Ireland	Netherlands	Sweden	US
Canada	Germany	Italy	New Zealand	Switzerland	